

Improving LC-MS Selectivity for Mesalamine Using Differential Ion Mobility Technology

Using the SCIEX Triple Quad™ 5500 LC-MS/MS System with SelexION® Technology

Anoop Kumar and Manoj Pillai
SCIEX, India

Selectivity and sensitivity are major considerations during the development of bioanalytical methods. In complex matrices, such as crashed human plasma, sometimes assays are affected by different challenges like isobaric matrix interference or high background noise. These would have an impact on both the sensitivity and reproducibility of the analyte at lower concentration in the calibration curve, due to poor signal to noise.

Resolving the matrix interference and lowering the background noise in plasma can often require extensive sample preparation, causing increased time and cost of method development and use. SelexION Technology adds an orthogonal level of separation and selectivity prior to the instrument orifice and can often be used reduce these interfering issues.

In the present study, the capability of SelexION technology coupled with MRM analysis was evaluated for use in the bioanalysis of Mesalamine in human plasma sample.



Key Feature of DMS for Mesalamine Quantitation

- SelexION Technology is a planar differential mobility separation device (DMS) that separates compounds based on differences in chemical and structural properties (Figure 1).
- SelexION Technology is compatible with the fast cycle times required for monitoring multiple MRM transitions or when using fast HPLC gradients.
- Use of DMS improved selectivity of the mesalamine assay by reducing the background interferences and improving the signal to noise ration
 - Signal to noise ratio was improved ~2X using DMS in human plasma.
- An LLOQ of 10 ng/mL for mesalamine was achieved using protein precipitated extraction method in human plasma.



Figure 1. SelexION® Technology. The DMS interface is directly coupled to the orifice plate. A modified curtain plate accommodates the DMS cell which can be easily installed and removed without the use of any tools and without venting the system. The source extension ring enables use of the standard SCIEX sources.

Methods

Sample Preparation: Plasma samples were spiked with Mesalamine and deuterated internal standard solution. The samples were derivatized with propionic anhydride at room temperature. Protein precipitation was performed, then the organic phase was collected and evaporated to dryness under nitrogen stream. The residue was finally reconstituted in mobile phase for analysis.

Chromatography: The samples were analyzed using the Shimadzu LC system. Chromatographic resolution was achieved on Kromasil C18 (4.6 x 150 mm column, 3.5 μm). Analyte elution was carried out using 5mM ammonium formate (pH 3.0) and methanol (35:65). Total run time was optimized to 6 min. Injection Volume was 10 μL.

Mass Spectrometry: Sample analysis was performed on a SCIEX Triple Quad™ 5500 system equipped with SelexION® device using a Turbo V™ source in positive electrospray mode. DMS parameters for Mesalamine were optimized in T infusion mode for the interest to maximize signal intensity and reduce the background interference. The optimized DMS settings are shown in Table 1. Data was acquired using Analyst® 1.6 Software.

Data Processing: Data was processed using MultiQuant™ Software.

Table 1. Optimized Differential Mobility Separation Settings.

Parameter	Setting
DMS Temperature	Medium
Modifier	None
Separation Voltage (SV)	3900
Compensation Voltage (CoV)	8.7
DMO Offset (DMO)	-8.0
DMS Resolution (DR)	Off

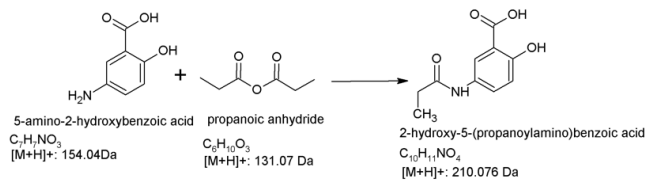


Figure 2. Derivatization Scheme of Mesalamine with Propionic Anhydride.

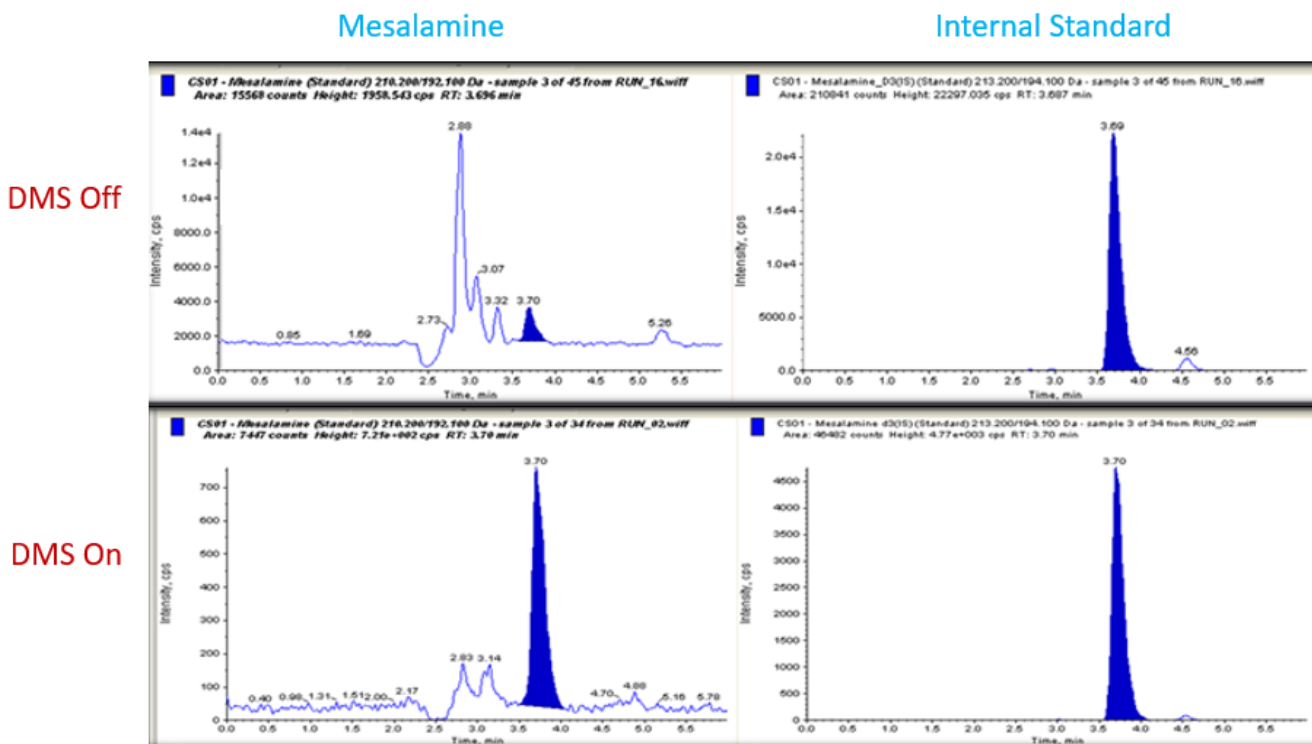


Figure 2. Analysis of Mesalamine in Human Plasma with and without DMS Separation.

Quantitation of Mesalamine in Human Plasma

The mesalamine method was developed using positive electrospray ionization. Mesalamine was derivatized using propionic anhydride to achieve the best sensitivity under room temperature. Protein precipitation was also used because it has less sample preparation steps and it is cost effective. During the method development, many background inference peaks were observed. Therefore, it was decided to determine if differential mobility separation would improve selectivity of the method. DMS separation parameters were optimized for the derivatized mesalamine (Table 1).

Use of SelexION technology significantly improved the signal to noise (~2X) by reducing the background noise in plasma samples (Figure 2). A linear calibration curve was constructed using the $1/X^2$ regression. The calibration curve for Mesalamine was linear over a dynamic range of 10.0 – 702 .0 ng/mL in plasma sample (Figure 3) with an r value 0.9998. Two precision and accuracy batches were processed to evaluate the developed method. Results of Mesalamine for precision and accuracy in batch-1 were given in Table 2. Different QCs level samples (n = 6) were also evaluated for precision and accuracy along with the calibration curve.

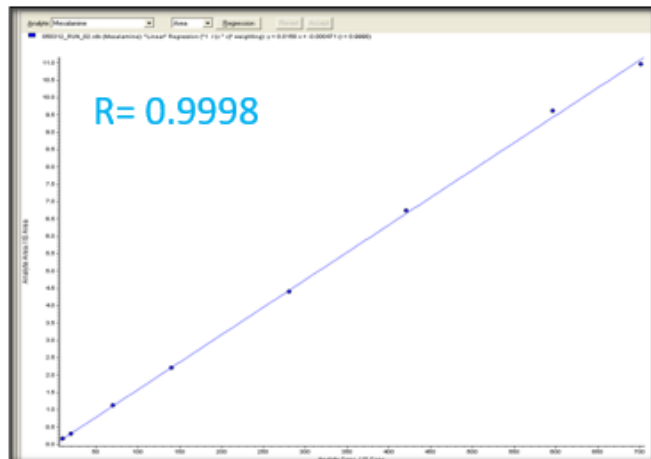


Figure 3. Calibration Curve of Mesalamine in Human Plasma from 10.0-702 ng/mL using SelexION Technology Separation.

The Mesalamine eluted at 3.70 min in a 6 min isocratic chromatographic run time. The signal to noise ratio of Mesalamine at LLOQ (10.0 ng/mL) in plasma is 14.2 calculated using sigma standard deviation of the baseline (Figure 4).

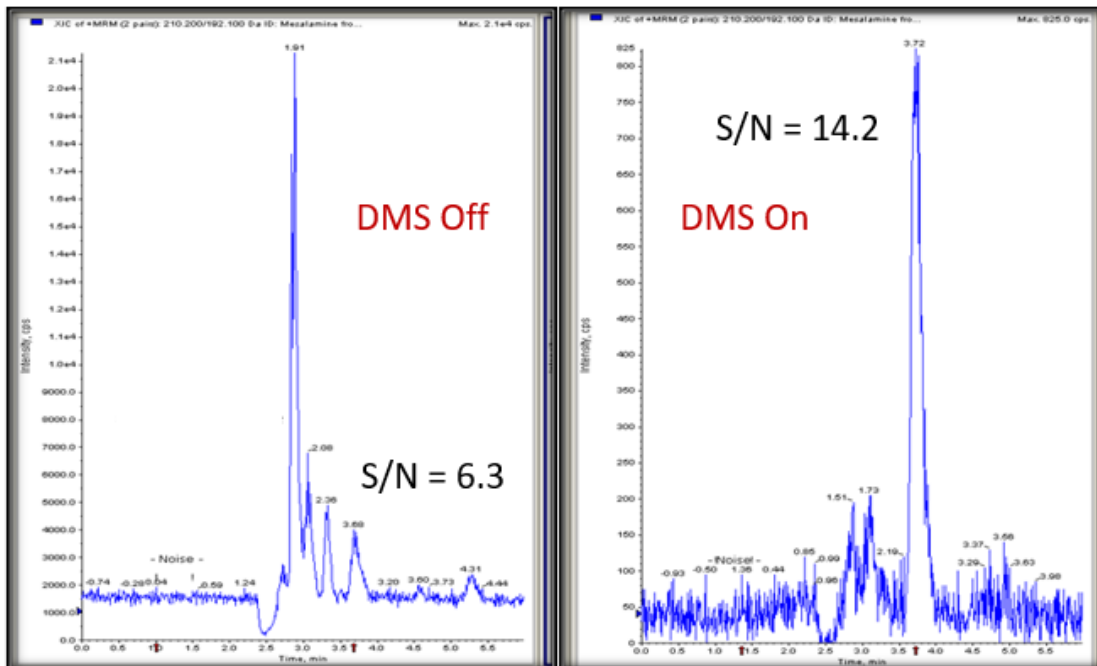


Figure 4. Signal to Noise Ratio of Mesalamine at LOQ Level in Plasma with and Without DMS Separation.

Conclusions

- Differential Mobility Separation (DMS) using SelexION Technology provides an orthogonal level of selectivity by separating components and interfering ions based on their chemical properties and ion mobility.
- Matrix interference and background noise for the mesalamine was significantly reduced to improve selectivity and thus improved the signal to noise ratio.
 - Signal to noise ratio was improved ~2X using DMS in human plasma.
- An LLOQ of 10 ng/mL for mesalamine was achieved using protein precipitated extraction method in human plasma.
- Precision and accuracy batch data for quality control (QCs) samples were meeting the requirements for regulated bioanalytical labs.

Table 1. Precision and Accuracy Statistics for the Quality Control Samples for Mesalamine in Plasma using SelexION Technology.

Data	LLQC	LQC	MQC	HQC
<i>Expected Concentration</i>	10	30.1	246	526
<i># of Values</i>	6 of 6	6 of 6	6 of 6	6 of 6
<i>Means</i>	10.0203	29.3450	251.2695	531.5597
<i>Std. Dev.</i>	0.6389	0.6569	5.5114	23.5638
<i>%CV</i>	6.37	2.23	2.19	4.43
<i>Accuracy</i>	100.2	97.49	102.14	101.05

Reference:

- SelexION® Technology: A New Solution to Selectivity Challenges in Quantitative Analysis. SCIEX Technical note RUO-MKT-02-3251-A.
- A Sensitive and Selective LC-differential mobility – mass spectrometric analysis of allopregnanolone and pregnanolone in human plasma. *Anal Bioanal Chem* (2013) **405**: 9497-9508.
- Planar differential mobility spectrometer as a pre-filter for atmospheric pressure ionisation mass spectrometry. (2010). *International Journal of Mass Spectrometry*. **298(1-3)**: 45-54.

AB Sciex is doing business as SCIEX.

© 2018 AB Sciex. For Research Use Only. Not for use in diagnostic procedures. The trademarks mentioned herein are the property of AB Sciex Pte. Ltd. or their respective owners. AB SCIEX™ is being used under license.

Document number: RUO-MKT-02-6491-B



Headquarters
500 Old Connecticut Path | Framingham, MA 01701 USA
Phone 508-383-7700
sciex.com

International Sales
For our office locations please call the division headquarters or refer to our website at sciex.com/offices