

# Analysis of PFAS in drinking water with EPA Method 537.1 and the SCIEX QTRAP® 4500 System


## Achieving 537.1 method requirements in a robust 10-minute method

Simon Roberts, Craig Butt, Dan Wright, Stephen Somerville, KC Hyland, Chris Borton  
 SCIEX, Redwood City, CA  
 EQI, Columbia, SC

In the United States, EPA method 537.1 describes the sample preparation, reporting guidelines, and quality control for the analysis of a suite of 14 per- and polyfluorinated substances (PFAS) in drinking water. The EPA 537.1 method guidelines provide some flexibility in the liquid chromatography tandem mass spectrometry (LC-MS/MS) analysis. Within these guidelines, optimization of certain aspects of the method, such as column chemistry, chromatography, mobile phases, gradient profile, and MS/MS transitions, was performed. Sample preservation and preparation guidelines published in EPA 537.1 are prescriptive and were therefore closely followed.

**Table 1. Names, abbreviations, and method detection limits (MDLs) for 14 PFAS compounds included in EPA Method 537.1 along with the reporting limits (MRLs) published by the UCMR3 guidelines 6 of the PFAS compounds. MDLs and MRLs shown as ng/L (ppt) here.**

Compound	Abbreviation	Method Detection Limit (ng/L)	UCMR3 Reporting Limit (ng/L)
Perfluorohexane carboxylate	PFHxA	0.09	-
Perfluoroheptane carboxylate	PFHpA	0.1	10
Perfluorooctane carboxylate	PFOA	0.1	20
Perfluorononane carboxylate	PFNA	0.09	20
Perfluorodecane carboxylate	PFDA	0.1	-
Perfluoroundecane carboxylate	PFUnDA	0.1	-
Perfluorododecane carboxylate	PFDoA	0.1	-
Perfluorotridecane carboxylate	PFTTrDA	0.2	-
Perfluorotetradecane carboxylate	PFTeDA	0.2	-
Perfluorobutane sulfonate	PFBS	0.1	90
Perfluorohexane sulfonate	PFHxS	0.08	30
Perfluorooctane sulfonate	PFOS	0.1	40
<i>n</i> -ethyl perfluorooctane sulfonamidoacetic acid	<i>n</i> -EtFOSAA	0.1	-
<i>n</i> -methyl perfluorooctane sulfonamidoacetic acid	<i>n</i> -MeFOSAA	0.09	-

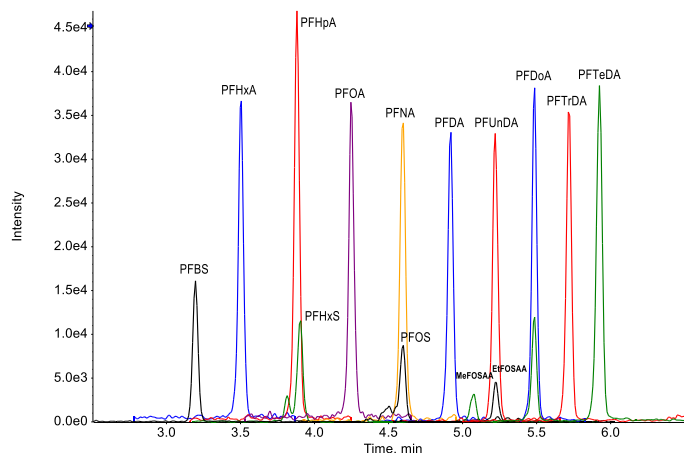

**Figure 1. PFAS standard mix at 50 ng/L (ppt) containing all 14 compounds in EPA 537.1 eluting within 6 minutes for an 11 minute total run time with a 10 uL injection.**

## Key Features of PFAS Analysis on the SCIEX QTRAP® 4500 System

- Robust and reproducible results with qualifying accuracy and precision for calculated concentrations, asymmetry factor, and linearity
- Total sample runtime takes only 8-10 min, depending on autosampler settings and system dead volume
- Sensitive MDLs of 0.08-0.2 ng/L for the entire suite of 14 PFAS compounds

## Sample Preparation

Sample preservation and preparation were performed according to the guidelines in EPA Method 537.1. Briefly, 1 g of Trizma was added to 250 mL polypropylene bottles. Bottles were pre-weighed to calculate the mass of sample collected. Surrogate standards were added to the sample container to achieve a final concentration of 2 ng/L in the 250 mL water sample.

The water samples were extracted using the following procedure with Phenomenex Strata-XL solid phase extraction cartridges (6 mL, 500 mg):

- 1) Condition SPE tubes with 15 mL of water followed by 18 mL of methanol
- 2) Add sample to tubes at a flow rate of approximately 10-15 mL per minute.
- 3) Rinse tubes with 7.5 mL of water and repeat
- 4) Dry tubes under vacuum for 5 minutes
- 5) Rinse sample bottle with 4 mL of methanol and transfer methanol to SPE tube while collecting eluent and repeat
- 6) Evaporate sample to dryness under nitrogen at 40-60°C
- 7) Reconstitute sample in 1 mL of 96% methanol 4% water containing 1 ng/L of internal standards
- 8) Transfer a 0.25 mL aliquot to a polypropylene vial and archive the remaining volume

## Liquid Chromatography

An Agilent 1200 binary pump was modified by replacing all clear fluoroethylene polymer (FEP) tubing with 1/8 in or 1/16 inch PEEK tubing. A delay column was inserted between the gradient mixing chamber and the autosampler valve to retain contaminants from the eluents or pumps for an extra 1-2 min compared with target analytes eluting from the analytical column.

**Table 2: Delay column and analytical HPLC columns from Phenomenex**

Column	Name	Dimensions
Delay column	Phenomenex Luna C18(2)	5 $\mu$ m; 30 x 2 mm
Analytical column	Phenomenex Gemini C18	3 $\mu$ m; 50 x 2 mm

An Agilent 1200 autosampler injected 10  $\mu$ l of each sample onto the analytical column (Phenomenex Gemini C18), which was heated to 40°C. Gradient separation was performed at a flow rate of 0.6 mL/min using the gradient shown in Table 3.

**Table 2: Gradient program**

Time (min)	A% (20 mM ammonium acetate)	B% (methanol)
0	95	5
0.1	45	55
4.5	1	99
8	1	99
8.5	95	5

## Mass Spectrometry

Samples were ionized using negative mode electrospray at the source conditions shown in Table 3 and the Q1/Q3 masses, declustering potentials, and collision energies shown in Appendix Table 1.

**Table 2: Source gas, temperature, and voltage settings**


Parameter	Value
CAD	9
CUR	30
GS1	40
GS2	60
IS Voltage	-4500
TEM	450

Calibration was performed using an 8-point curve at concentrations of 50, 100, 200, 500, 1000, 2000, 5000, and 10000 ng/L and the concentrations of surrogates and internal standards was 1,000 ng/L in all final sample extracts, standards, method blanks, and quality control samples. Quantitation was performed using MultiQuant™ 3.0.2 using 1.0 point Gaussian smoothing and 1/x weighted linear regression forced through the origin (as required by EPA 537.1). A concentration factor of 250 was applied to samples as a result of the concentration of 250 mL to the final 1 mL extract.

## Results

The initial calibration achieved the following guidelines prescribed in EPA method 537.1:

- 1) Linearity ( $r^2 > 0.99$ ) (as shown in Figure 2)
- 2) Accuracy ( $\pm 30\%$  for each calibrator)
- 3) Precision (RSD  $< 20\%$  of 4 replicates of a fortified blank)
- 4) Asymmetry factor ( $> 0.8$  and  $< 1.5$  for the first 2 peaks in the chromatogram as shown in Figure 3)
- 5) Surrogate recovery  $\pm 30\%$  of expected response
- 6) Laboratory reagent blanks (LFBs) and field reagent blanks (FRBs) quantitated at  $< 1/3$  of the MRL.

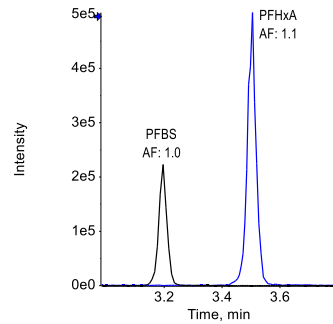


**Figure 3: Asymmetry factor (AF) calculated for the first 2 eluting peaks, PFBS and PFHxA, at a mid-point standard concentration of 500 ng/L**

After 8 days of analyzing samples to calculate the MDL and other samples, the continuing calibrations still met the requirements of  $\pm 30\%$  of expected calculated concentration for all 14 analytes, as shown in Table 4.


**Table 4: Accuracy of a 50 ng/L calibration standard injected immediately after the initial calibration curve and 6 and 8 days after the calibration curve.**

Compound	Days after Calibration			Accuracy (%)		
	0	6	8	0	6	8
PFBS	44.8	54.6	57.7	90%	109%	115%
PFHxA	54.8	52.2	52.6	110%	104%	105%
PFHpA	55.1	50.4	58.0	110%	101%	116%
PFHxS	47.1	53.9	49.3	94%	108%	99%
PFOA	52.2	58.9	53.7	104%	118%	107%
PFNA	55.1	50.9	51.3	110%	102%	103%
PFOS	47.0	45.5	48.7	94%	91%	97%
PFDA	52.7	53.5	52.3	105%	107%	105%
PFUdA	52.9	48.5	52.9	106%	97%	106%
PFDoA	54.5	56.9	55.0	109%	114%	110%
PFTTrDA	52.0	54.8	51.5	104%	110%	103%
PFTeDA	51.6	51.0	53.0	103%	102%	106%
n-EtFOSAA	55.7	53.9	57.2	111%	108%	114%
n-MeFOSAA	56.7	61.6	58.2	113%	123%	116%

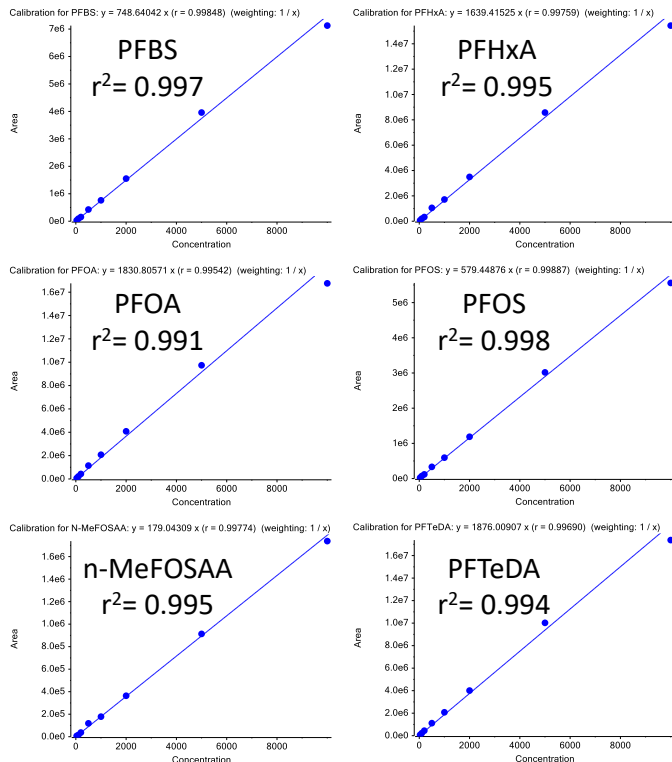


**Figure 3: Linearity of 6 of the PFASs analyzed out of the suite of 14 showing  $r^2 > 0.99$  with a linear fit forced through the origin and  $1/x$  concentration weighting. The other 8 PFAS compounds also showed  $r^2 > 0.99$ .**

To calculate method detection limits, 9 water samples were spiked with approximately 0.2 ng/L of each of the 14 PFAS compounds and analyzed following the full analytical protocol. The calculated MDLs shown Figure 1 were calculated according to EPA 537.1 using the mean and standard deviation of the replicated spiked samples. The MDLs for all 14 compounds was below 0.2 ng/L, which highlights the excellent sensitivity of the method.

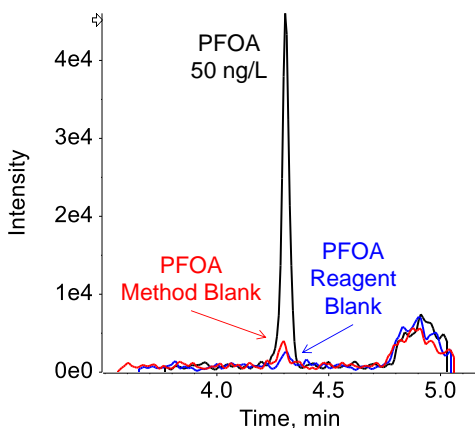

**Figure 5: Blank chromatograms showing extremely low contamination in blank samples compared with the 50 ng/L calibration standard. The small peak at 4.9 min is the PFOA contamination eluting from the delay column, which originates from the HPLC pumps and eluent.**

Blank samples showed very low responses and were always below the requirement of  $<1/3$  of the MRL. Figure 5 shows the response of a method blank (red), which was a 250 mL water sample taken through the entire sample preparation protocol, and a reagent blank, which was 96% methanol and 4% water prepared in an autosampler vial. A small peak at 4.9 min in the chromatogram in Figure 5 shows presence of PFOA contamination presumably in the HPLC pumps or eluents and demonstrates the adequate separation from the quantitated analyte peak as a result of the delay column installment.

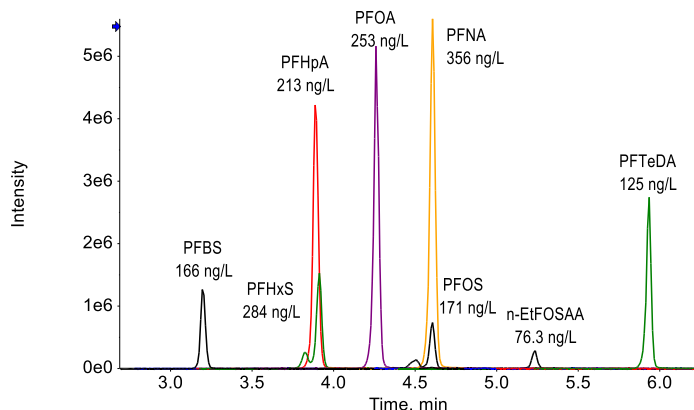

**Figure 6: Proficiency testing samples were run to establish method performance met EPA requirements.**

PT samples were obtained from ERA and were analyzed along with the MDL replicates. The PT samples were diluted 10:1 with water and analyzed according to the procedures described in this note. The results of the 8 analytes present in PT CAT: 960 were all within  $\pm 18\%$  of the assigned concentration of the PT study.

The HPLC method and MS/MS analysis for this validated 537 method were both fully compatible with an extended list of 25 analytes. However, the EPA method 537 sample preparation protocol relies on reverse phase, hydrophobic interactions for solid phase extraction (SPE) retention and, therefore, fails to adequately retain shorter chain PFCAs, including perfluorobutane carboxylate and perfluoropentane carboxylate. Modifying this sample preparation method by replacing Strata-XL with Strata-XL-AW (weak anion exchange) solid phase extraction tubes and altering the solvents used during extraction allows a longer, extended list to be analyzed using the same method.

## Conclusions

Robust and reproducible results with qualifying accuracy and precision for calculated concentrations, asymmetry factor, and linearity were achieved in a single ten-minute LC-MS/MS acquisition on the SCIEX QTRAP® 4500 system. Following stringent protocols for sample preparation and preservation defined by the EPA 537.1 method, method optimization steps were taken to continue to improve PFAS analysis workflow and quantitative performance. Background contamination was minimized through LC system adjustments (replacing FEP tubing and installing delay column). Analysis of shorter-chain PFCAs was improved through selection of weak anion exchange sorbent for sample SPE. Sensitive MDLs of 0.08-0.2 ng/L for the entire suite of 14 PFAS compounds were achieved, all of which meet or exceed the requirements of the US EPA's UCMR3 list for drinking water, and method robustness was demonstrated by sustained accuracy of measured concentration in a QC sample over eight days without need for re-injection of calibration standards.

**Appendix Table 1. MRM transitions, instrument voltage parameters, and retention times.**

Name	Q1	Q3	RT (min)	DP	CE	Name	Q1	Q3	RT (min)	DP	CE
PFBS	298.9	80	3.2	-20	-56	13C8_PFOS	507	80	4.7	-20	-95
PFBS_2	298.9	99	3.2	-20	-46	PFDA	513	469	5	-10	-17
13C3_PFBS	302	80	3.2	-20	-56	PFDA_2	513	169	5	-10	-27
PFHxA	313	269	3.5	-10	-14	13C2_PFDA	515	470	5	-10	-17
PFHxA_2	313	119	3.5	-10	-25	13C6_PFDA	519	474	5	-10	-16
13C2_PFHxA	315	270	3.5	-10	-14	PFUdA	563	519	5.3	-10	-18
13C5_PFHxA	318	273	3.5	-10	-14	PFUdA_2	563	169	5.3	-10	-28
PFHpA	363	319	3.9	-10	-14	13C7_PFUdA	570	525	5.3	-10	-18
PFHpA_2	363	169	3.9	-10	-25	N-MeFOSAA	570	419	5.2	-50	-28
13C4_PFHpA	367	322	3.9	-10	-14	N-MeFOSAA_2	570	483	5.2	-50	-22
PFHxS	399	80	3.9	-20	-74	d3-MeFOSAA	573	419	5.2	-50	-28
PFHxS_2	399	99	3.9	-20	-60	N-EtFOSAA	584	419	5.3	-50	-28
13C3_PFHxS	402	80	3.9	-20	-74	N-EtFOSAA_2	584	526	5.3	-50	-28
PFOA	413	369	4.3	-10	-14	d5-EtFOSAA	589	419	5.3	-50	-28
PFOA_2	413	169	4.3	-10	-26	PFDoA	613	569	5.6	-10	-18
13C2_PFOA	415	370	4.3	-10	-14						
13C8_PFOA	421	376	4.3	-10	-14						
PFNA	463	419	4.7	-10	-16						
PFNA_2	463	169	4.7	-10	-26						
13C9_PFNA	472	427	4.7	-10	-16						
PFOS	499	80	4.7	-20	-95						
PFOS_2	499	99	4.7	-20	-87						
13C4_PFOS	503	80	4.7	-20	-95						

AB Sciex is doing business as SCIEX.

© 2018 AB Sciex. For Research Use Only. Not for use in diagnostic procedures. The trademarks mentioned herein are the property of AB Sciex Pte. Ltd. or their respective owners. AB SCIEX™ is being used under license.

Document number: RUO-MKT-02-7657-A



**Headquarters**  
 500 Old Connecticut Path | Framingham, MA 01701 USA  
 Phone 508-383-7700  
[sciex.com](http://sciex.com)

**International Sales**  
 For our office locations please call the division  
 headquarters or refer to our website at  
[sciex.com/offices](http://sciex.com/offices)